MIDMARK®

Installation/Operation Instructions

9A83001 INSTRUMENT TRAY

KIT COMPONENTS

Part Number	Description	Qty.
9A83001	Instrument Tray	1
003-0936-00	Installation / Operation Instructions	1

REQUIRED TOOLS

None

INTRODUCTION

To hold instruments for an examination or general procedure.

WARNING

Must be mounted on base rail of exam table. Must be removed or rotated clear of moving parts before positioning table. Always support Instrument Tray when changing positions on it. Assure all positions are solidly locked to prevent movement during procedure.

INSTALLATION

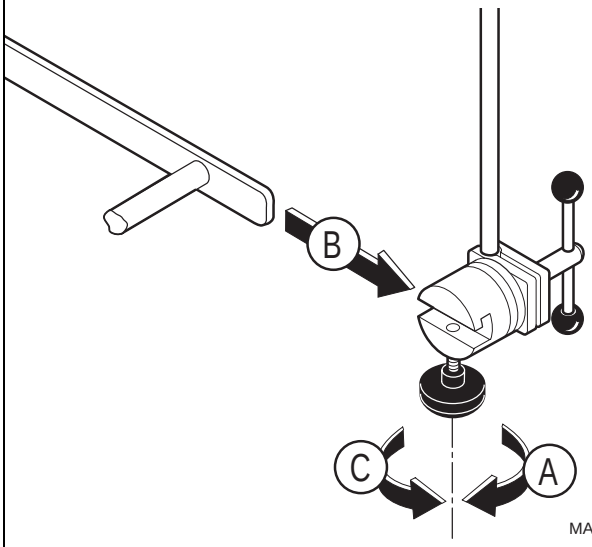

EQUIPMENT ALERT

Place table in desired position before mounting 9A83001 Instrument Tray. Do not operate the table after the Tray has been installed to prevent damage to the table or Tray.

A. Loosen knob.
B. Slide swivel block onto side rail to desired position.
C. Tighten knob.

OPERATION (ROTATIONAL POSITIONING)

NOTE

The Instrument Tray can be rotated two ways.

1.

A. Supporting Instrument Tray, loosen handle
B. Rotate Tray to desired position.
C. Tighten handle.

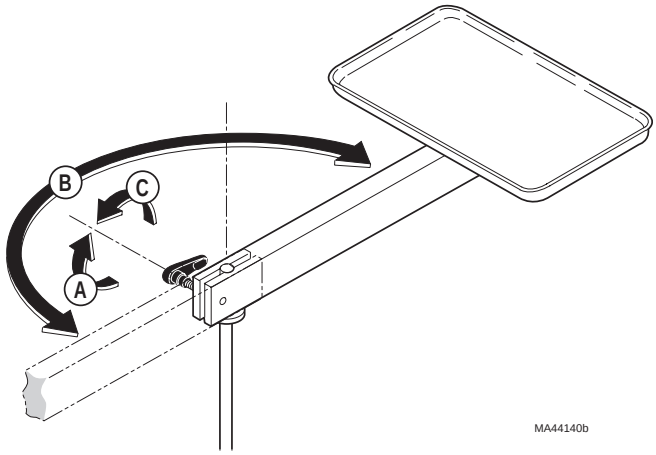

2.

A. Loosen handle.
B. Rotate Tray.
C. Tighten handle.

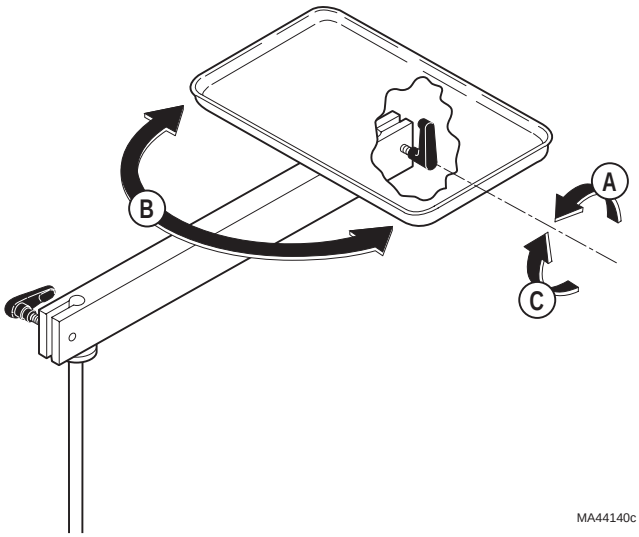

© Midmark Corporation - 1998

OPERATION
(HEIGHT ADJUSTMENT)

A. SupportingTray, loosen T-handle.
B. Raise or lower Tray.
C. Tighten T-handle.

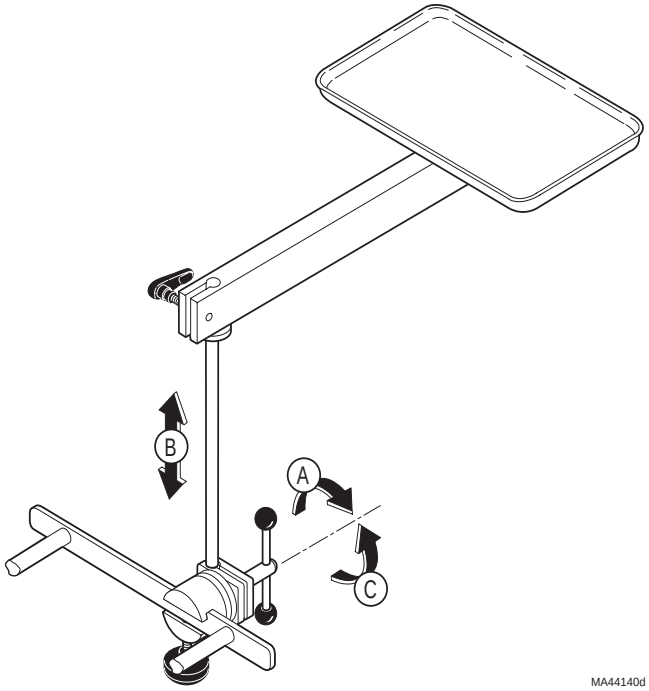

MIDMARK®
Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

© Midmark Corporation - 1998